



European Organisation  
for Astronomical  
Research in the  
Southern Hemisphere

Organisation Européenne  
pour des Recherches  
Astronomiques  
dans l'Hémisphère Austral

Europäische Organisation  
für astronomische  
Forschung in der  
südlichen Hemisphäre

# **VERY LARGE TELESCOPE**

## **X-shooter Imaging Mode Manual and A&G CCD Characteristics**

Date: 14/06/2014

Version: 2nd release v1 P94

Authors: C. Martayan, A. Mehner, G. Beccari, E. Pena, W. Hummel, A. Modigliani,  
A. Smette, and the X-shooter IOT

## CHANGELOG

Version-Period-Date	Sections	Comments
v1-P93 27/11+16/12/2013	All	1st version, warning this is a preliminary release, some information is still missing and will come with the commissioning in January 2014.
22/01/2014	2	Small changes for some values after commissioning
14/06/2014	2, 3, 4, 5, 7	-Reference added -correction of detector values -new section about stability measurements -fringing maps added -New templates added

### Glossary:

A&G or AG: acquisition and guiding

DEC: declination

ETC: exposure time calculator

OB: observing block

RA: right ascension

RMS: root mean square

RON: readout noise

SM: service mode

TCCD: technical CCD

VM: visitor mode

ZP: zeropoint

<b><u>1.</u> Overview</b>	p4
<b><u>2.</u> Detector characteristics, filters, and zeropoints</b>	p5
<b><u>3.</u> Stability</b>	p9
<b><u>4.</u> Calibration plan</b>	p10
<b><u>5.</u> Distortion map, fringes, and astrometric accuracy</b>	p13
<b><u>6.</u> Frames overview and examples</b>	p16
<b><u>7.</u> Data reduction guidelines</b>	p18
<b><u>8.</u> Templates manual</b>	p20

### **Acknowledgements:**

We kindly ask you to cite the following article (exact reference to come soon) if you use the X-shooter images:

*The X-shooter Imaging Mode*  
*Martayan et al., The Messenger, 156, June 2014*

In addition this document provides complementary information to this manual and we recommend its reading.

### **Contact:**


user support department:  
usd-help at eso.org  
usd\_xshooter at eso.org

# 1. Overview

X-shooter remains foremost a set of spectrographs, but a simple imaging mode with limited functionalities is offered to the community starting in P93. The imaging mode uses the 4th arm of X-shooter that corresponds to the Acquisition and Guiding (A&G) camera and its set of filters (see Figure 1). Acquisition images have already been used in past periods to obtain reference photometry to flux calibrate spectra in addition to the usual spectrophotometric observations. Other applications have been the determination of magnitudes of transient objects such as GRB counterparts, supernovae, and variable objects (e.g., stellar binaries and stars with exoplanets).

With the implementation of the imaging mode in P93 only one acquisition snapshot will be saved (and not after each applied offset as was previously the case). For direct target acquisition one snapshot will be saved once the acquisition process is finished. In case of a target acquisition using a blind offset one snapshot will be saved at the end of the acquisition of the reference star and one after the blind offset is performed.

Figure 1: Schematic overview of X-shooter.

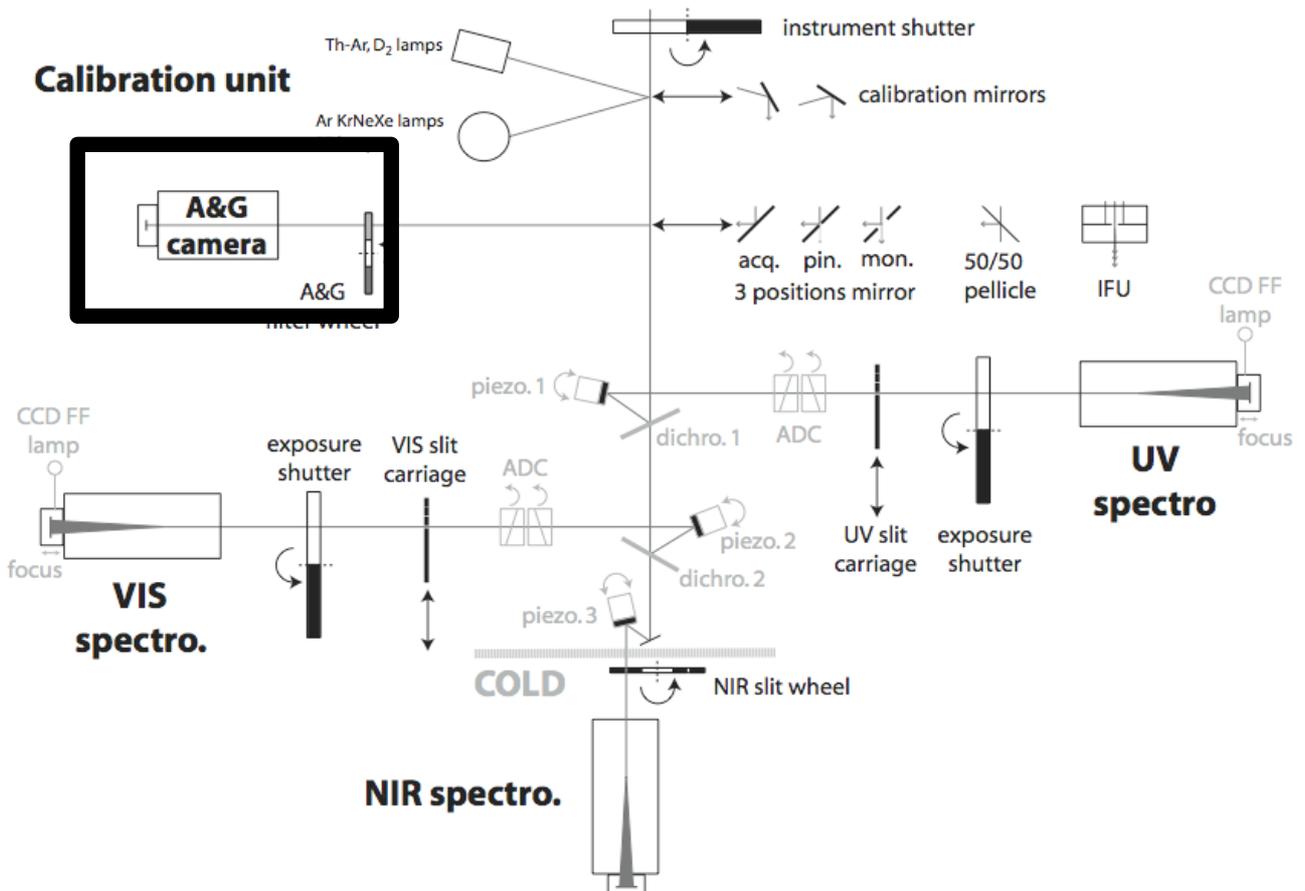

## 2. Detector characteristics, filters, and zeropoints

The A&G unit consists of:


- A Pelletier cooled, 13  $\mu\text{m}$  pixel, 512x512 E2V broad band coated Technical CCD57-10 onto which the focal plane is re-imaged at f/1.91 through a focal reducer. This setup provides a plate scale of 0.174"/pix and a field of view of 1.47'x1.47'.
- A filter wheel equipped with a full UBVRI Johnson filter set and a full Sloan Digital Sky Survey (SDSS) filter set.

Table 1: A&G CCD characteristics.

<b>Detector type</b>	E2V CCD57-10IE
<b>Cooling system</b>	Pelletier
<b>QE</b>	82 % at 580 nm, 50 % at 380 nm and 820 nm
<b>Number of pixels</b>	562x528
<b>Pixel size</b>	13 $\mu\text{m}$ x13 $\mu\text{m}$
<b>Pixel scale ("/pixel)</b>	0.1744 +/- 0.0016 (since P92 at UT3)
<b>Field of view</b>	1.5'x1.5' (but filters do not cover the corners)
<b>Gain (e-/ADU)</b>	1.29 $\pm$ 0.02
<b>Readout noise (e- rms)</b>	4.14 $\pm$ 0.08
<b>Saturation (ADU)</b>	65535
<b>Readout mode and overheads</b>	Fast readout mode only. Wipe time: 0.01 s, readout time: 0.33 s, transfer time: 0.78 s, total time: 1.12 s.
<b>Dark current level (ADU/pixel/h)</b>	0.97 (exposure time of 10s)
<b>Fringing amplitude</b>	Not characterized yet. Depends on the filters. 2 to 4 % in l, z'
<b>Non-linearity (ADU)</b>	<1 % at 10000 and 50000 ADUs
<b>Bias level (ADU)</b>	1688 $\pm$ 5.5
<b>Prescan and overscan areas</b>	X: 1-26 and 538-562 Y: 1-15 and 528

Figure 2: A&G CCD quantum efficiency curve.

### A&G Camera CCD

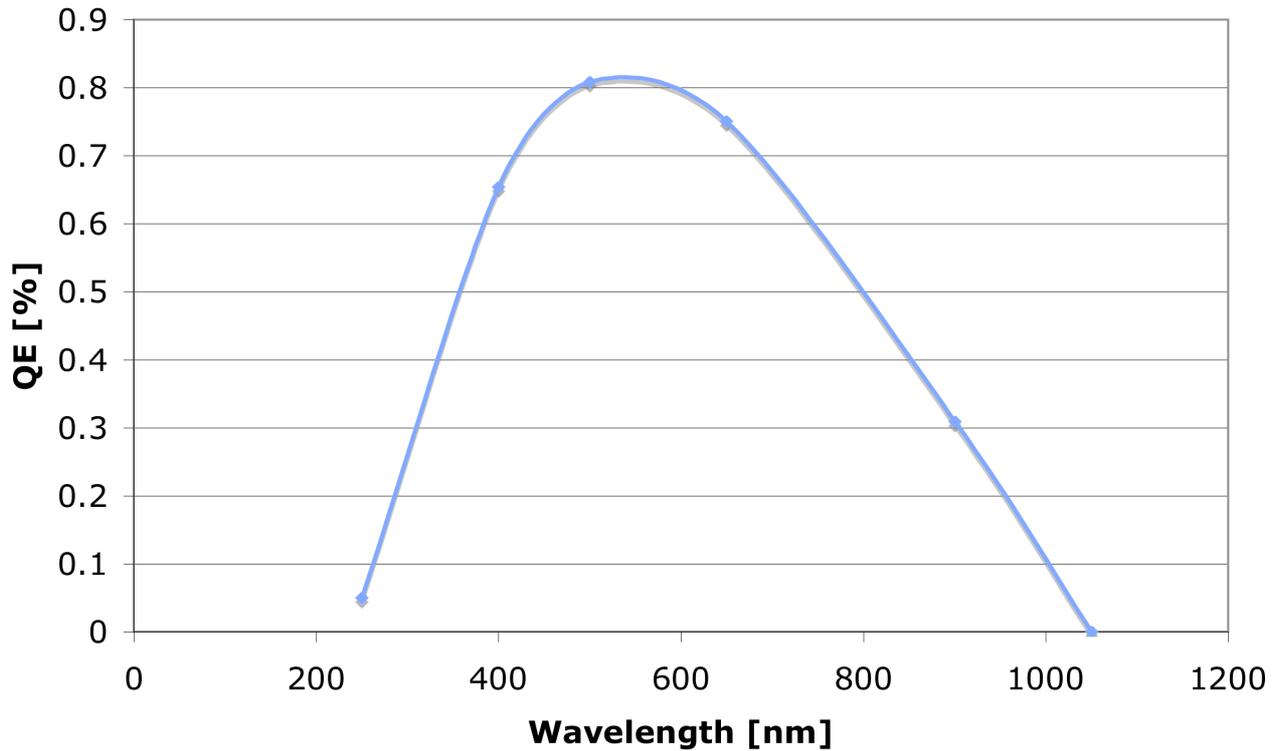

The A&G CCD cooling system produces small oscillations of the CCD temperature. Temperature variations affect the dark current level. In case of short exposure times, when the image sampling frequency corresponds to the frequency of the temperature oscillations, this leads to “beats” and background level variations from one image to the next. These variations in background level disappear if a longer exposure time is selected. However, they do not affect the acquisition performance. In June 2011, the noise was improved and the quality of images now allows to detect objects as faint as magnitudes 25 in R and V bands in 3 min exposures and good weather conditions.

Figure 3: A&G camera filter curves.

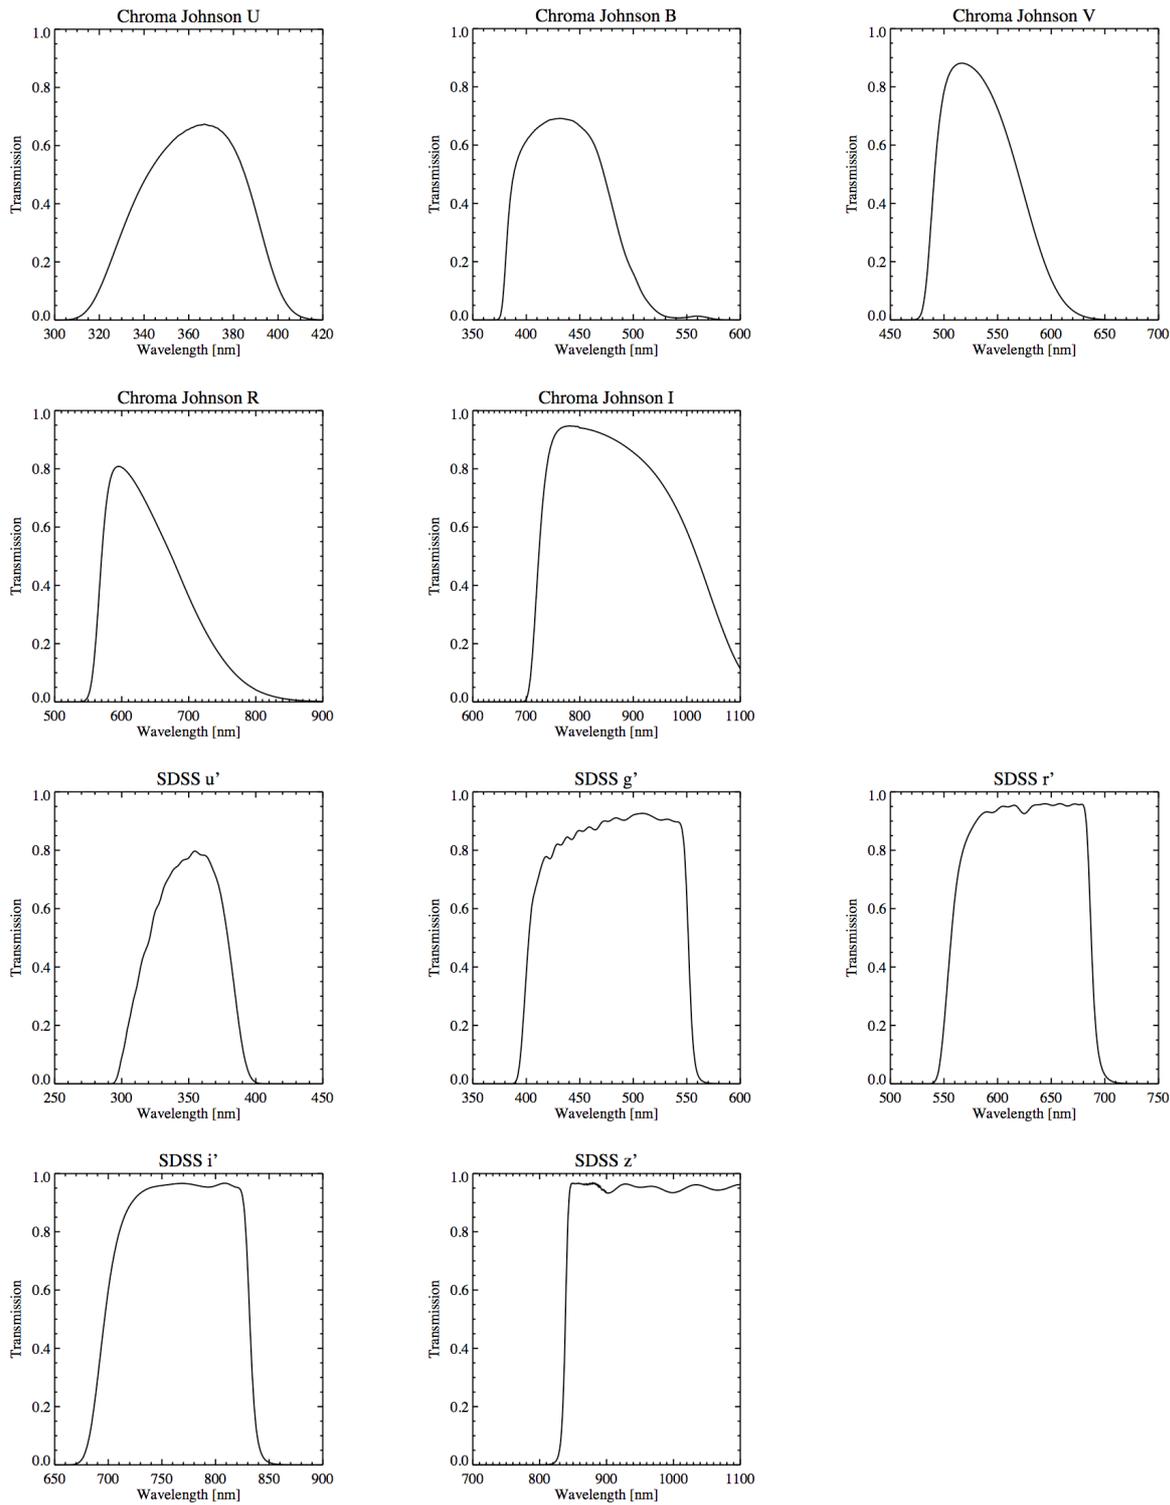


Table 2: A&G CCD zeropoints.

	U	B	V	R	I
ZP XSHOOTER (11/2013) at UT3 from P92	24.83	27.91	27.83	27.74	27.36
ZP XSHOOTER (07/2011) at UT2 till P91	24.95	27.74	27.63	27.83	27.49
ZP FORS2	24.31	27.68	28.09	28.32	27.67


Note: The A&G CCD zeropoints were determined for the Johnson filters under photometric condition. The accuracy of the ZP X-shooter magnitudes determined with at UT3 are about 0.1 mag, at UT2 about 0.1-0.3 mag depending on the filters. FORS2 zeropoints are shown for comparison.

### 3. Stability


The stability of the imaging mode and the AG CCD detector was investigated. Short, medium and long term stability aspects were tested.

a) The spectrophotometric standard star GD71 was monitored over 1 hour with exposures every few seconds. The 1-s standard deviation in B and V bands are 0.006 magnitude for both band. It represents a variation of 0.4%.

b) The stability at medium term was checked with the evolution of the bias and readout noise levels. They are shown below. Over a period of 52 days, the RMS of the bias level variability is 0.33% and for the RON it is 0.56%.

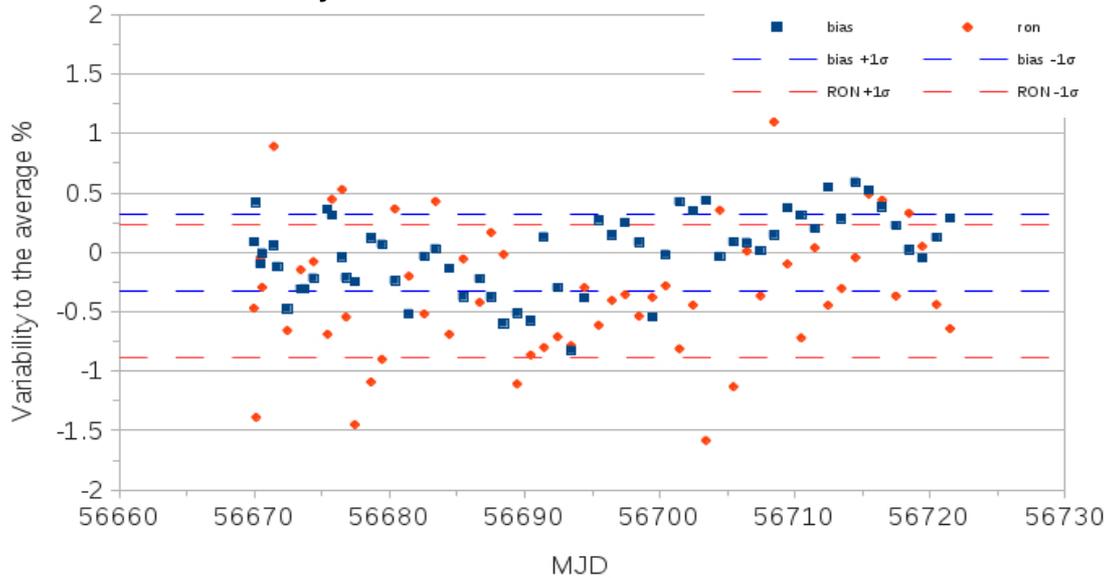

c) the long term stability of the instrument was tested with the spectrophotometric standard star EG274 observed during a period of more than 500 days, However, the star was quite often observed under sub-optimal condition (twilight with fast variable sky background, etc). Nevertheless, the RMS is of 0.42% over 1.4 years.

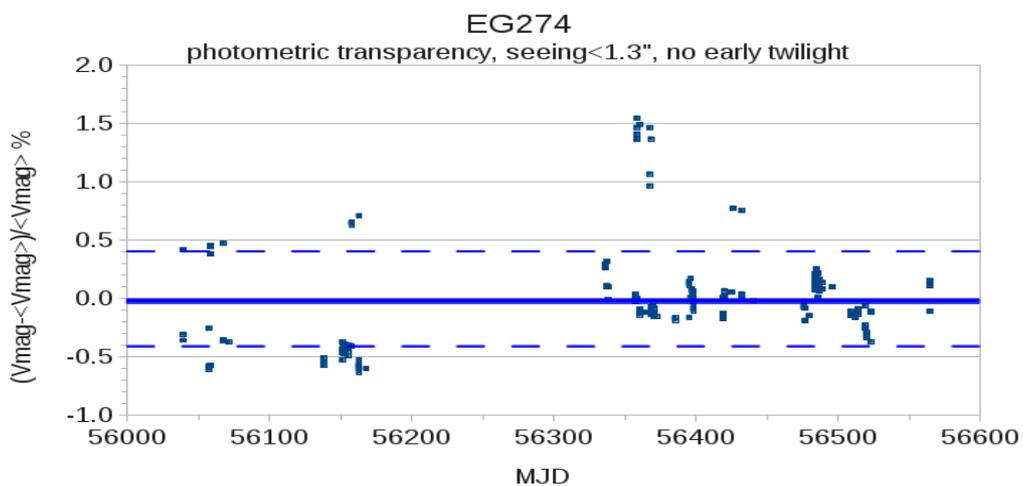

## 4. Calibration plan and observing strategies

### a) Imaging mode acquisition and exposure times

A basic imaging observing block (OB) consists of a slit or IFU acquisition template, followed by science and/or calibration imaging templates. However, pure imaging OBs are approved only in visitor mode. Exceptions in service mode are observations of standard fields for zeropoint determination or distortion maps. In service mode, OBs can contain imaging templates in addition to the standard slit or IFU science spectral templates.

There is no ETC support for the imaging mode. We recommend to scale the exposures times using the limiting magnitudes listed in Table 3. These magnitudes were obtained under relatively bad weather conditions (thin cirrus, full Moon, seeing about 0.7").

*Those 2 paragraphs mostly concern the spectroscopic acquisition but are kept for information.*

*Table 3 lists recommended exposure times for a set of magnitudes. These integration times should suffice for a direct acquisition in case of clear sky conditions, dark time, and 0.8" seeing. However, in case of very faint objects, a blind offset acquisition is the best solution as it shortens the acquisition overheads.*

Table 3: Limiting magnitudes for a direct acquisition.

U	B	V	R	I
22	22	22.5	22.5	22.5
30 s	30 s	20 s	20 s	20 s

*The table 4 already provides few clues about S/N and exposure times. We recommend to use blind offset acquisitions in case the object is fainter than 22-22.5 mag, especially if relaxed weather constraints were selected such as thin/thick transparency and seeing worse than 0.7". In case of a blind offset acquisition, we recommend to select a reference star with a magnitude of 19 mag or brighter to ensure good centering.*

Table 4: Recommended exposure times for the A&G CCD (S/N>5).

V (mag)	6	7	16-20	23	≥24
Exposure time (s)	0.001	0.005	1-5	60-120	≥180

## b) Observing strategies

Two science templates are offered:


1. *XSHOOTER\_img\_obs*: STARE mode observation, i.e., the object stays on the same detector pixel.
2. *XSHOOTER\_img\_obs\_GenericOffset*: GENERIC-OFFSET mode observations, i.e., mapping or jittering around the area of interest.

Table 5: Imaging science templates.

	Templates	Readout speed and binning	List of filters	Angles
IMAGING	STARE GENERIC-OFFSET	Fast readout, binning 1x1	U,B,V,R,I, u',g',r',i',z'	9999=parallactic angle or defined angle on sky

It is recommended to use the *XSHOOTER\_img\_obs\_GenericOffset* template. This template results in better correction of the sky background and the dust spots visible in the detector. One can define a sequence of small offsets as shown in the following example. Offsets are given in arcsec, but the reference system can be chosen to be the sky (Alpha,Delta) or X-shooter detector coordinate system (X,Y). Offset conventions are illustrated below. Templates use **cumulative offsets**; the position at a given time is derived from the *sum* of all offsets specified so far in the template. For example, the series of offsets: 0, -10, 0, 10 brings the telescope back to the original position for the last exposure.

Figure 4: Offset example.

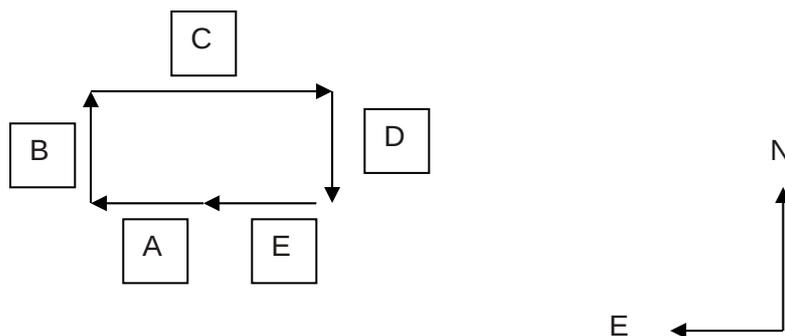

Note: Offsets A = (RA = +10", DEC = 0"); B = (RA = 0", DEC = +10"); C = (RA = -20", DEC = 0"); D = (RA = 0", DEC = -10"); E = (RA = +10", DEC = 0") bring the telescope back to the original position.

### c) Calibration plan

The calibration plan is defined below. It may evolve in the next months/periods.

Table 6: Calibration plan.

Type of calibration	Template	Frequency
Day: bias	XSHOOTER_img_cal_Dark	10, daily
Day: dark	XSHOOTER_img_cal_Dark	on request, 3x10s monthly
Day: linearity	XSHOOTER_img_cal_DetLin	monthly
Night: twilight flats	XSHOOTER_img_cal_Flat	10, monthly*
Night: zeropoints	XSHOOTER_img_obs_cal_phot	once per year or user provided
Night: distortion map	XSHOOTER_img_obs_cal_dist	once per year or user provided

\*The count levels of the twilight flats should be between 10000 and 55000 ADUs. In P93 they will be taken pointing to empty sky positions while until P92 they are taken at the zenith (thus star traces may be possible).

### d) Quality control

Some health check plots of the AGCCD are available at:

[http://www.eso.org/observing/dfo/quality/XSHOOTER/reports/HEALTH/trend\\_report\\_BIAS\\_AGC\\_HC.html](http://www.eso.org/observing/dfo/quality/XSHOOTER/reports/HEALTH/trend_report_BIAS_AGC_HC.html)


the bias level, the readout noise, the noise structure, the dark current are monitored.


The linearity and gain are also monitored but there is no plot yet available.

## 5. Distortion map, fringes, and astrometric accuracy

Figure 5 shows the distortion maps of the TCCD with respect to the 2MASS astrometry.


Figure 5: UBVR I distortion maps magnified x20.

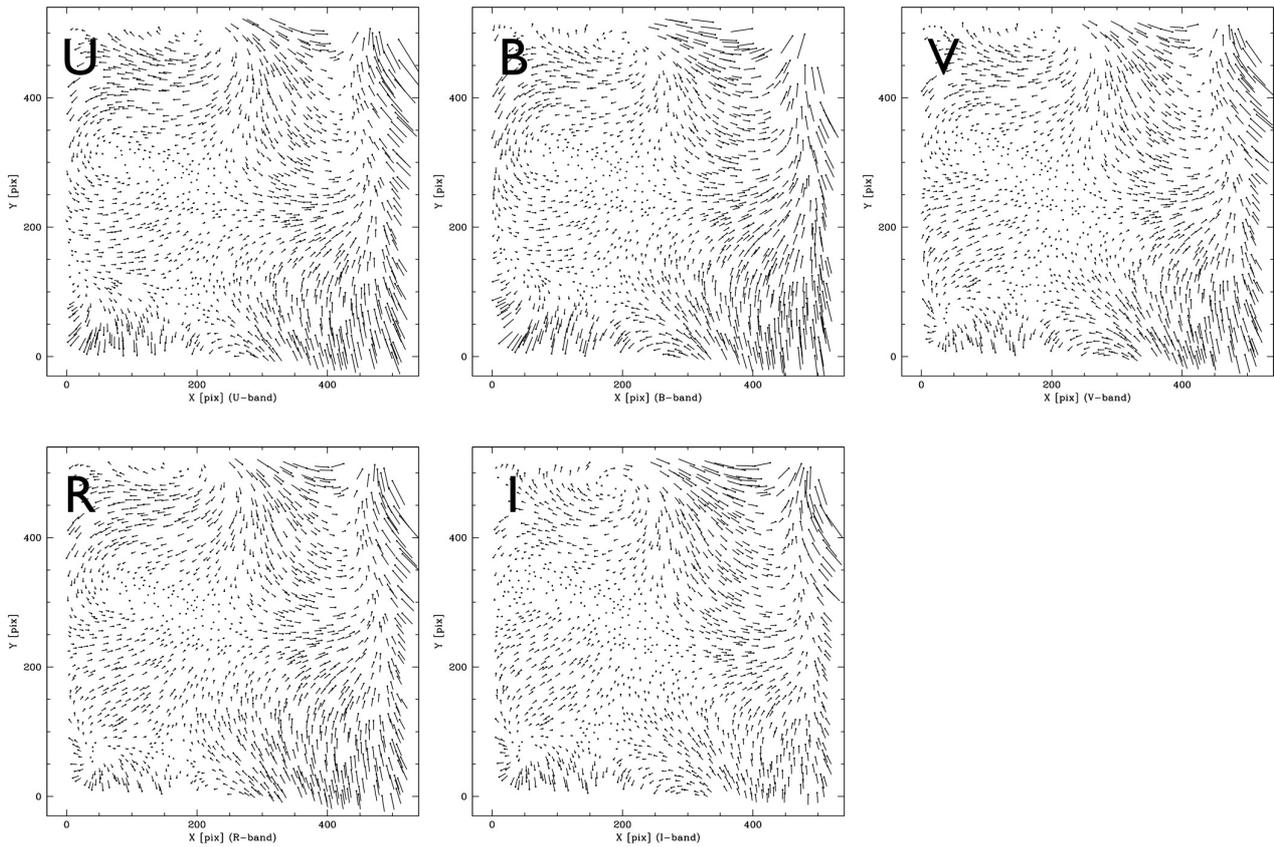


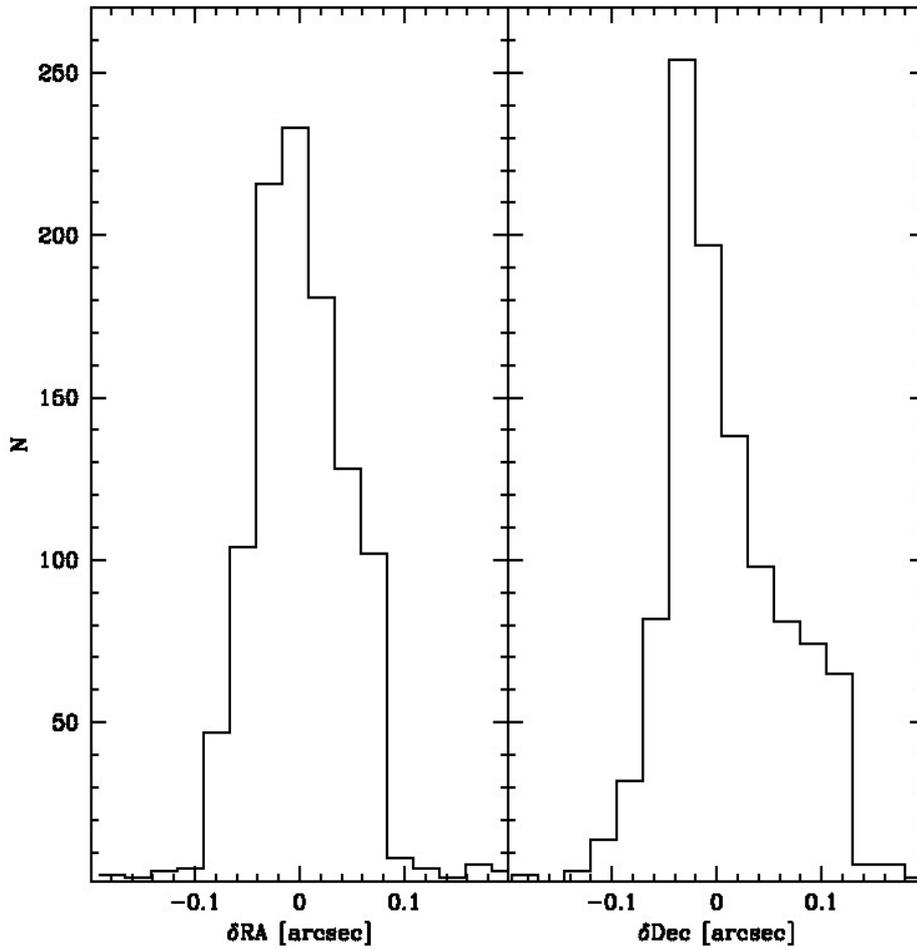


Distributions in RA and DEC of the difference between 2MASS and the AGCCD astrometry. The difference between 2MASS and the A&G CCD astrometry is  $\pm 0.1''$ .


**The Fringing maps** were obtained with skyflats.  
The most affected filters are the r', i', z', l.  
The amplitude peak to peak ranges from 2 % in the r' to 4% in the z' filter.

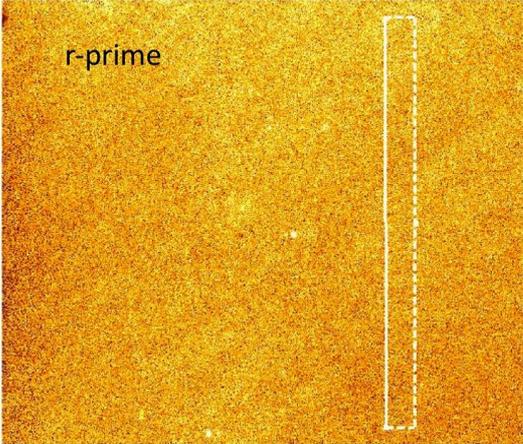

Projection

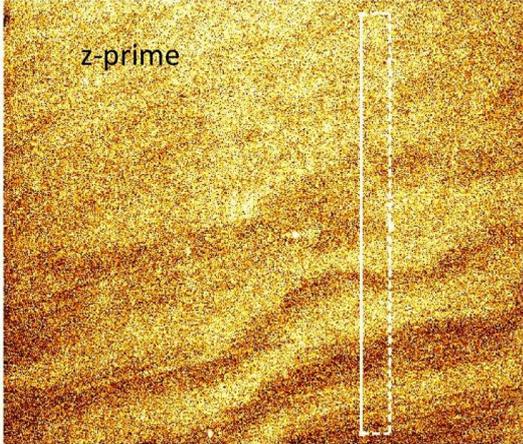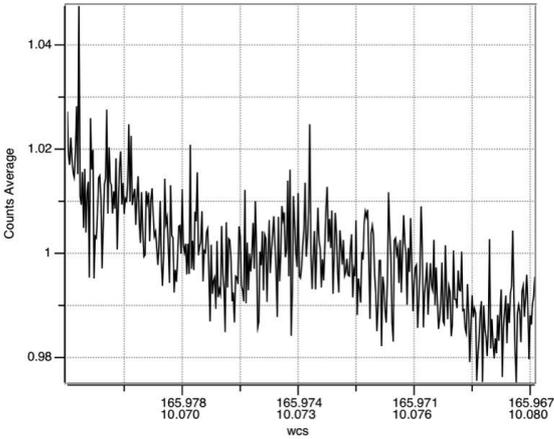


Projection

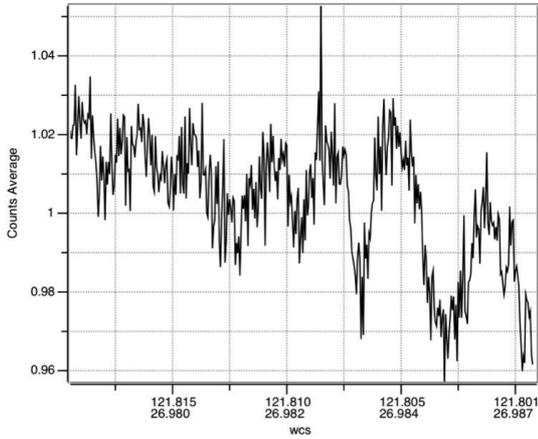


## **6. Calibration frames overview and examples**

Figure 6: Three color (BVI) image of a galaxy with a supernova (left) and of a small field of 47Tuc (right).

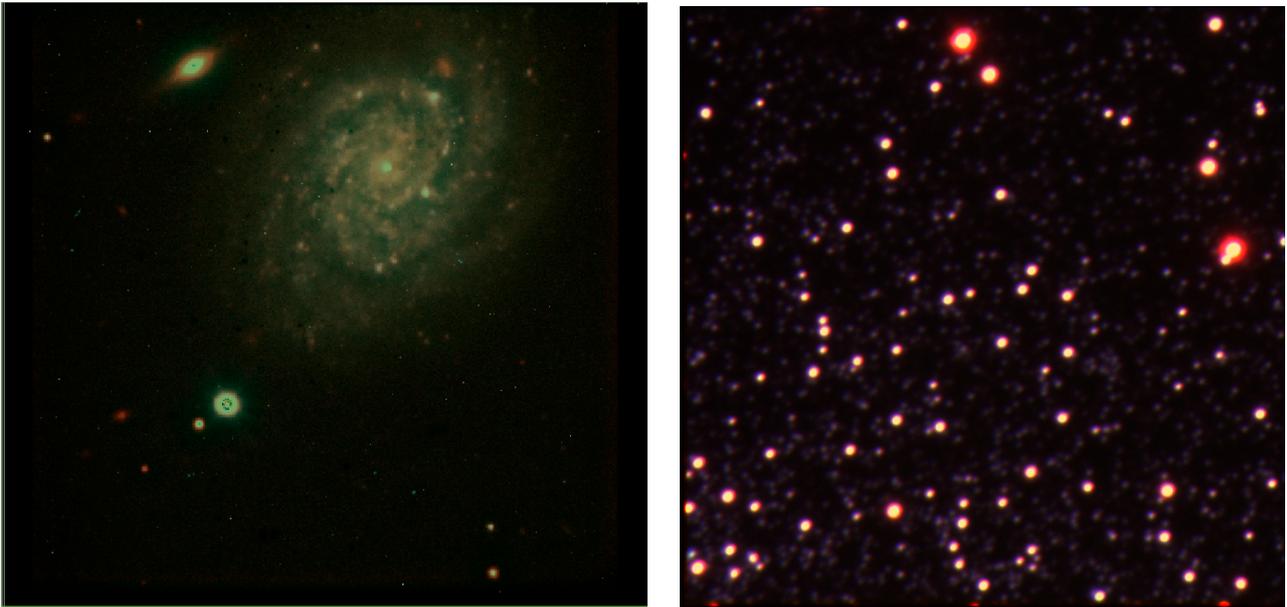


Observations were performed in stare mode.  
More examples are shown in the Messenger article of the XSHOOTER imaging mode.

Figure 7: Example of calibration images.

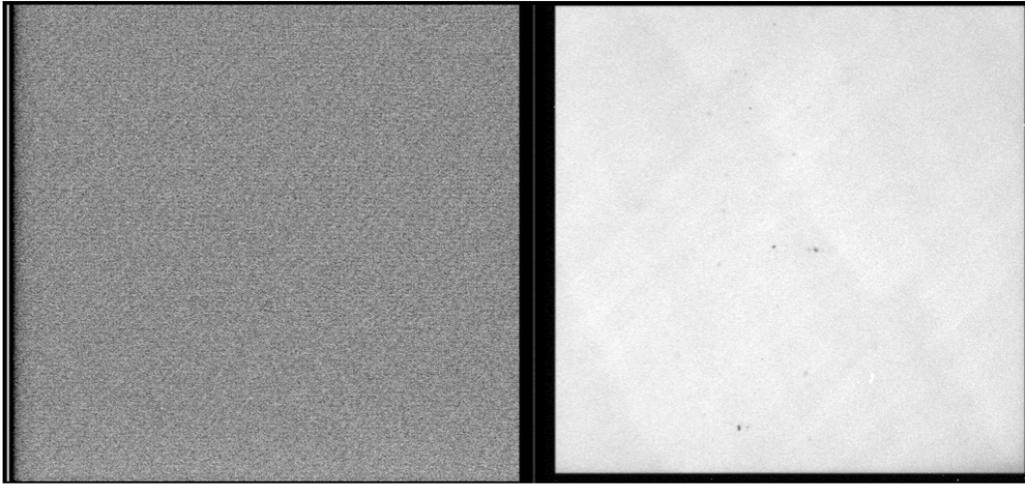


A&G CCD bias.

A&G CCD twilight U band flatfield.

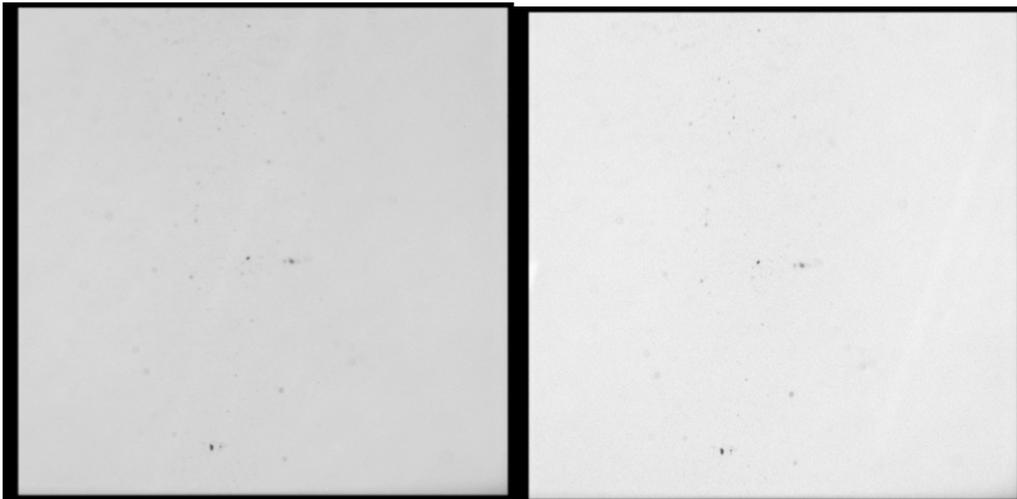

A&G CCD twilight B band flatfield.

A&G CCD twilight V band flatfield.

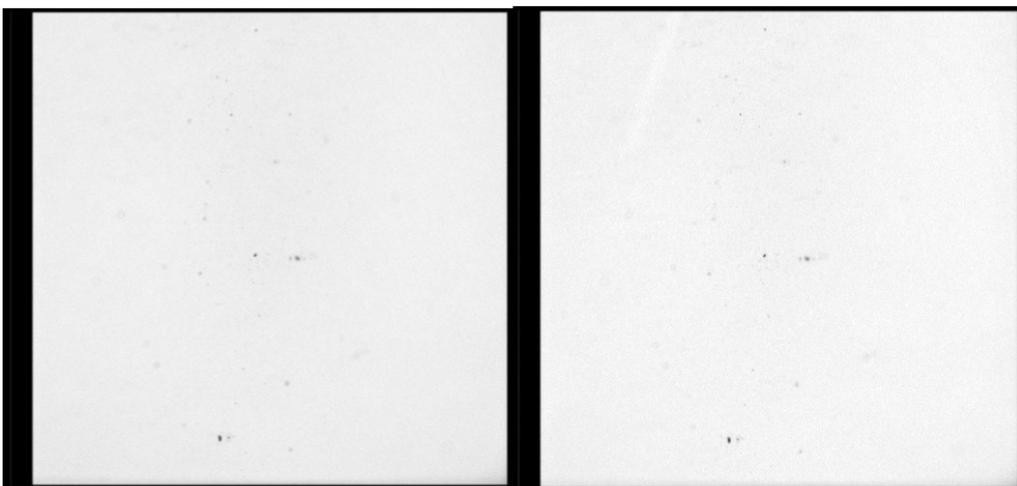

A&G CCD twilight R band flatfield.

A&G CCD twilight I band flatfield.

## 7. Data reduction

No pipeline support will be provided for the imaging data as there are lots of tools to reduce imaging data, extract the objects, and do the photometry. Pipeline support will be provided for the detector linearity determination only. Below are some basic guidelines of imaging data reduction with IRAF and the swarp software:

### 0) Preliminary steps

- Inspect the images, reject the flat-fields with too many stars or star traces.
- Create files listing the frames per type.
- Make sure to use darks and flatfields with the same integration times.

### 1) Create the masterbias

- In IRAF, use the imcombine task to median combine the bias images.



```
cmartayan@nb015045:~/duties/xshooter/moveUT2to...
IRAF
Image Reduction and Analysis Facility
PACKAGE = immatch
TASK = imcombine

input = [] @listebias List of images to combine
output = masterbias.fits List of output images
(headers= ) List of header files (optional)
(bpmasks= ) List of bad pixel masks (optional)
(rejmask= ) List of rejection masks (optional)
(nrejmas= ) List of number rejected masks (optional)
(expmask= ) List of exposure masks (optional)
(sigmas = ) List of sigma images (optional)
(imcmb = $!) Keyword for IMCMB keywords
(logfile= STDOUT) Log file

(combine= median) Type of combine operation
(reject = minmax) Type of rejection
(project= no) Project highest dimension of input images?
(outtype= real) Output image pixel datatype
(outlimi= ) Output limits (x1 x2 y1 y2 ...)
(offsets= none) Input image offsets
(masktyp= none) Mask type
(maskval= 0) Mask value
(blank = 0.) Value if there are no pixels

(scale = none) Image scaling
(zero = none) Image zero point offset
(weight = none) Image weights
(statsec= ) Image section for computing statistics
(expname= ) Image header exposure time keyword

(lthresh= INDEF) Lower threshold
(hthresh= INDEF) Upper threshold
(nlow = 1) minmax: Number of low pixels to reject
(nhigh = 1) minmax: Number of high pixels to reject
(nkeep = 1) Minimum to keep (pos) or maximum to reject (neg)
(mclip = yes) Use median in sigma clipping algorithms?
(lsigma = 3.) Lower sigma clipping factor
(hsigma = 3.) Upper sigma clipping factor
(rdnoise= 0.) ccdclip: CCD readout noise (electrons)
(gain = 1.) ccdclip: CCD gain (electrons/DN)
(snoise = 0.) ccdclip: Sensitivity noise (fraction)
(sigscal= 0.1) Tolerance for sigma clipping scaling corrections
(pclip = -0.5) pclip: Percentile clipping parameter
(grow = 0.) Radius (pixels) for neighbor rejection
(mode = ql)
```

### 2) Optionally: create the masterdark


- Same than 1) for combining the images.

### 3) Create the masterflatfield

- Same than 1) for combining the images.
- Determine the count level with the IRAF imstat task.
- Normalize the image with the imarith task to obtain the master flatfield.

#### 4) Correct the science images for bias, dark, and flatfield

- Use the imarith task.

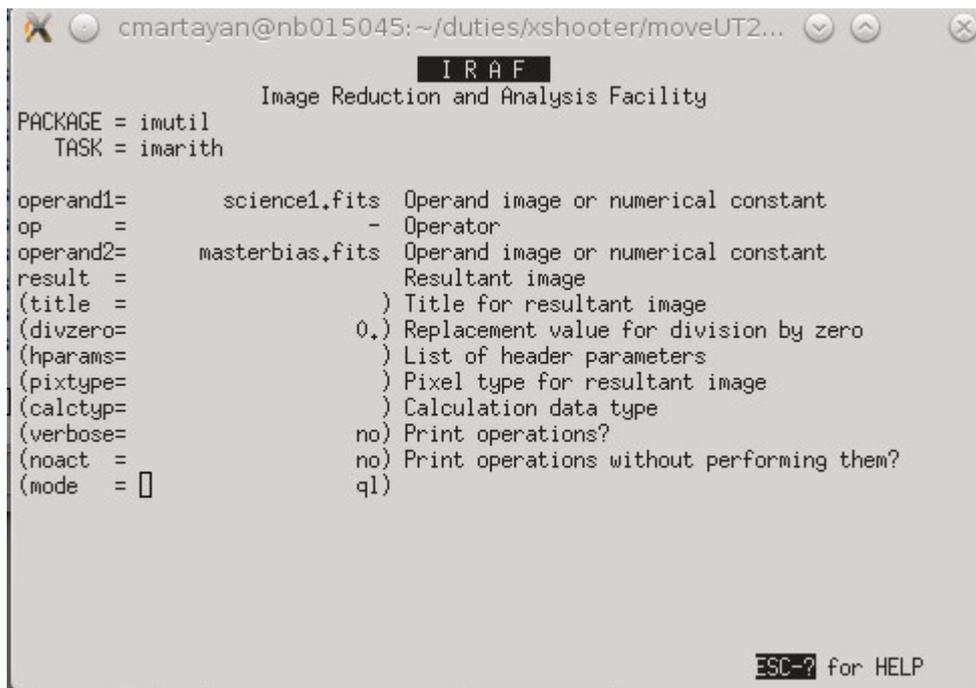

```
cmartayan@nb015045:~/duties/xshooter/moveUT2...
I R A F
Image Reduction and Analysis Facility
PACKAGE = imutil
TASK = imarith

operand1=      science1.fits  Operand image or numerical constant
op            =      -        Operator
operand2=      masterbias.fits Operand image or numerical constant
result       =
(title       =      ) Title for resultant image
(divzero     =      0.) Replacement value for division by zero
(hparams    =      ) List of header parameters
(pixtype    =      ) Pixel type for resultant image
(calctyp    =      ) Calculation data type
(verbose     =      no) Print operations?
(noact      =      no) Print operations without performing them?
(mode       =      []

ESC-? for HELP
```

#### 5) Stack the science images WCS based: use swarp

It is possible to use the IRAF tasks imstack or imcombine to combine the science images. However, it has been shown that IRAF does not always properly handle large images or the WCS. Therefore, we recommend to use the swarp software from astromatic (ex-TERAPIX) from E. Bertin (<http://www.astromatic.net/software/swarp>).

Syntax:

```
swarp @liste_files_images -c configuration_file
```

the configuration\_file contains all the parameters needed for the creation of the mosaic taking into account the WCS and recomputing it.

In the file liste\_files\_images: list all images that are needed for the mosaic.

## 8. Templates manual

### a) Approved template combinations

VM only	<p>XSHOOTER_img_acq+</p> <p>XSHOOTER_img_obs, XSHOOTER_img_obs_GenericOffset</p>
SM	<p>XSHOOTER_img_acq+</p> <p>XSHOOTER_img_cal_phot and/or XSHOOTER_img_cal_dist</p>
	<p>XSHOOTER_slt_acq* + 1 SLT science or std template</p> <p>Possibility to add:</p> <p>XSHOOTER_img_obs, XSHOOTER_img_obs_GenericOffset, XSHOOTER_img_cal_phot, XSHOOTER_img_cal_dist</p>
	<p>XSHOOTER_ifu_acq* + 1 IFU science or std template</p> <p>Possibility to add:</p> <p>XSHOOTER_img_obs, XSHOOTER_img_obs_GenericOffset, XSHOOTER_img_cal_phot, XSHOOTER_img_cal_dist</p>
	<p>XSHOOTER_img_acq_FlatSky.tsf + imaging skyflats templates</p> <p>Possibility to add:</p> <p>XSHOOTER_img_cal_Flat.tsf</p>

## b) Template description

### NIGHTTIME IMAGING TEMPLATES:

*Imaging acquisition template (also allows blind offset)*

XSHOOTER_img_acq.tsf			
<i>To be specified:</i>			
Parameter	Hidden	Range (Default)	Label
DET4.WIN1.UITI	no	0..36000 (1)	TCCD Exposure time
DPR.CATG	yes	(ACQUISITION)	Data Prod. Cath.
DPR.TECH	yes	(IMAGE)	Data Prod. Tech.
DPR.TYPE	yes	(OBJECT)	Data Prod. Type
INS.FILT1.NAME	no	u_prime g_prime r_prime i_prime z_prime U B V R I (V)	
G Filter			
SEQ.PRESET	yes	F T (T)	Preset flag
TEL.AG.GUIDESTAR	no	CATALOGUE SETUPFILE NONE (CATALOGUE)	Get Guide Star from
TEL.GS1.ALPHA	no	ra ( )	RA of guide star
TEL.GS1.DELTA	no	dec ( )	DEC of guide star
TEL.ROT.OFFANGLE	no	-179.99..179.99 9999.0 (9999.0)	Position Angle on Sky
TEL.TARG.ADDVELALPHA	yes	(0.0)	Additional Velocity RA in arcsec/s on the sky
TEL.TARG.ADDVELDELTA	yes	(0.0)	Additional Velocity DEC in arc- sec/s on the sky
TEL.TARG.ALPHA	no	ra (000000.000)	RA
TEL.TARG.DELTA	no	dec (000000.000)	DEC
TEL.TARG.EPOCH	no	1950 2000 (2000)	Epoch
TEL.TARG.EQUINOX	no	QUERY-TARG getEquinoxList (2000)	Equinox
TEL.TARG.OFFSETALPHA	no	-36000..36000 (0.)	Offset RA
TEL.TARG.OFFSETDELTA	no	-36000..36000 (0.)	Offset DEC
TEL.TARG.PMA	yes	-10..10 (0)	Proper motion in RA
TEL.TARG.PMD	yes	-10..10 (0)	Proper motion in DEC

---

Parameter	Hidden	Value	Label
-----------	--------	-------	-------

---

Special imaging acquisition template for taking imaging skyflats.  
 This template presets the telescope but does not request any active optics or  
 guiding. This template can be combined with the skyflats template:  
 XSHOOTER\_img\_cal\_Flat.tsf

XSHOOTER_img_acq_FlatSky.tsf			
To be specified:			
Parameter	Hidden	Range (Default)	Label
DET4.WIN1.UIT1	no	0..36000 (1)	TCCD Exposure time
DPR.CATG	yes	ACQUISITION SCIENCE CALIB TEST (ACQUISITION)	Data Prod. Cath.
DPR.TECH	yes	ECHELLE ECHELLE,IFU ECHELLE,IFU,OFFSET ECHELLE,IFU,STARE ECHELLE,SLIT ECHELLE,SLIT,OFFSET ECHELLE,SLIT,STARE ECHELLE,MULTI-PINHOLE ECHELLE,SLIT,NODDING	Data Prod. Tech.
DPR.TYPE	yes	IMAGE (IMAGE) OBJECT OB- JECT,OFFSET BIAS DARK FLAT,LINEARITY,DETCHAR FLAT,SKY LAMP,FLAT LAMP,ORDERDEF LAMP,AFC STD,FLUX STD,TELLURIC STD,ASTROMETRY STD,TELLURIC ARC (OBJECT)	Data Prod. Type
INS.FILT1.NAME	no	u_prime g_prime r_prime i_prime z_prime U B V R I (V)	
G Filter			
SEQ.PRESET	yes	F T (1)	Preset flag
TEL.AG.GUIDESTAR	no	CATALOGUE SETUPFILE NONE (CATALOGUE)	Get Guide Star from
TEL.GS1.ALPHA	no	ra (°)	RA of guide star
TEL.GS1.DELTA	no	dec (°)	DEC of guide star
TEL.ROT.OFFANGLE	no	-179.99..179.99 9999.0 (9999.0)	Position Angle on Sky
TEL.TARG.ADDVELALPHA	yes	(0.0)	Additional Velocity RA in arcsec/s on the sky
TEL.TARG.ADDVELDELTA	yes	(0.0)	Additional Velocity DEC in arc- sec/s on the sky
TEL.TARG.ALPHA	no	ra (000000.000)	RA
TEL.TARG.DELTA	no	dec (000000.000)	DEC
TEL.TARG.EPOCH	no	1950 2000 (2000)	Epoch
TEL.TARG.EQUINOX	no	QUERY-TARG getEquinoxList (2000)	Equinox
TEL.TARG.OFFSETALPHA	no	-36000..36000 (0.)	Offset RA
TEL.TARG.OFFSETDELTA	no	-36000..36000 (0.)	Offset DEC
TEL.TARG.PMA	yes	-10..10 (0)	Proper motion in RA
TEL.TARG.PMD	yes	-10..10 (0)	Proper motion in DEC
Parameter Hidden Value Label			

### Science STARE imaging observation

XSHOOTER_img_obs.tsf			
<i>To be specified:</i>			
Parameter	Hidden	Range (Default)	Label
DET4.WIN1.UIT1	no	0..36000 (1)	TCCD Exposure time
DPR.CATG	no	(SCIENCE)	Data Prod. Cath.
DPR.TECH	no	(IMAGE)	Data Prod. Tech.
DPR.TYPE	no	(OBJECT)	Data Prod. Type
INS.FILT1.NAME	no	u_prime g_prime r_prime i_prime z_prime U B V R I (V)	
G Filter			
SEQ.NEXPO	no	0..1000 (1)	Number of exposures

---

Parameter	Hidden	Value	Label

---

### Science Generic-OFFSET imaging observation

XSHOOTER_img_obs_GenericOffset.tsf			
<i>To be specified:</i>			
Parameter	Hidden	Range (Default)	Label
DET4.WIN1.UIT1	no	0..36000 (1)	TCCD Exposure time
DPR.CATG	yes	(SCIENCE)	Data Prod. Cath.
DPR.TECH	yes	(IMAGE)	Data Prod. Tech.
DPR.TYPE	yes	(OBJECT,OFFSET)	Data Prod. Type
INS.FILT1.NAME	no	u_prime g_prime r_prime i_prime z_prime U B V R I (V)	
G Filter			
SEQ.NEXPO	no	0..100 (1)	Number of exposures
SEQ.NOFFSET	no	1..100 (2)	Number of offsets
SEQ.OBS.TYPE	no	(O S)	List of TYPE offsets: e.g. O S S O
SEQ.OFFSET.COORDS	no	SKY DETECTOR (SKY)	O S ... Offset coord type (RA/DEC - X/Y) in arcsec
SEQ.OFFSET.ZERO	no	T F (T)	Go to zero offset position at the end
SEQ.RELOFF1	no	-1000..1000 (1)	List of RA/X offsets
SEQ.RELOFF2	no	-1000..1000 (1)	List of DEC/Y offsets

---

Parameter	Hidden	Value	Label

---

Calibration template for observation of standard field for distortion map  
(same functionality as the science imaging generic-offset template)

XSHOOTER_img_obs_cal_dist.tsf			
To be specified:			
Parameter	Hidden	Range (Default)	Label
DET4.WIN1.UIT1	no	0..36000 (1)	TCCD Exposure time
DPR.CATG	yes	(CALIB)	Data Prod. Cath.
DPR.TECH	yes	(IMAGE)	Data Prod. Tech.
DPR.TYPE	yes	(STD,ASTROMETRY)	Data Prod. Type
INS.FILT1.NAME	no	u_prime g_prime r_prime i_prime z_prime U B V R I (V)	
G Filter			
SEQ.NEXPO	no	0..100 (1)	Number of exposures
SEQ.NOFFSET	no	1..100 (2)	Number of offsets
SEQ.OBS.TYPE	no	(O S)	List of TYPE offsets: e.g. O S S O
SEQ.OFFSET.COORDS	no	SKY DETECTOR (SKY)	O S ... Offset coord type (RA/DEC - X/Y) in arcsec
SEQ.OFFSET.ZERO	no	T F (T)	Go to zero offset position at the end
SEQ.RELOFF1	no	-1000..1000 (1)	List of RA/X offsets
SEQ.RELOFF2	no	-1000..1000 (1)	List of DEC/Y offsets
Parameter Hidden Value Label			

Calibration template for observation of standard fields for zeropoint  
determination (same functionality as the science imaging generic-offset  
template)

XSHOOTER_img_obs_cal_phot.tsf			
To be specified:			
Parameter	Hidden	Range (Default)	Label
DET4.WIN1.UIT1	no	0..36000 (1)	TCCD Exposure time
DPR.CATG	yes	(CALIB)	Data Prod. Cath.
DPR.TECH	yes	(IMAGE)	Data Prod. Tech.
DPR.TYPE	yes	(STD,FLUX)	Data Prod. Type
INS.FILT1.NAME	no	u_prime g_prime r_prime i_prime z_prime U B V R I (V)	
G Filter			
SEQ.NEXPO	no	0..100 (1)	Number of exposures
SEQ.NOFFSET	no	1..100 (2)	Number of offsets
SEQ.OBS.TYPE	no	(O S)	List of TYPE offsets: e.g. O S S O
SEQ.OFFSET.COORDS	no	SKY DETECTOR (SKY)	O S ... Offset coord type (RA/DEC - X/Y) in arcsec
SEQ.OFFSET.ZERO	no	T F (T)	Go to zero offset position at the end
SEQ.RELOFF1	no	-1000..1000 (1)	List of RA/X offsets
SEQ.RELOFF2	no	-1000..1000 (1)	List of DEC/Y offsets
Parameter Hidden Value Label			

## DAYTIME IMAGING TEMPLATES

Calibration template for biases ( $DET4.WIN1.UIT1 = 0$  s) and darks ( $DET4.WIN1.UIT1 > 0$  s)

XSHOOTER_img_cal_Dark.tsf			
<i>To be specified:</i>			
Parameter	Hidden	Range (Default)	Label
<b>DET4.WIN1.UIT1</b>	no	0..36000 (1)	TCCD Exposure time
<b>DPR.CATG</b>	yes	(CALIB)	Data Prod. Cath.
<b>DPR.TECH</b>	yes	(IMAGE)	Data Prod. Tech.
<b>DPR.TYPE</b>	yes	(BIAS)	Data Prod. Type
<b>SEQ.NEXPO</b>	no	0..100 (1)	Number of exposures
<i>Fixed values:</i>			
Parameter	Hidden	Value	Label

Calibration template for twilight flatfields

XSHOOTER_img_cal_Flat.tsf			
<i>To be specified:</i>			
Parameter	Hidden	Range (Default)	Label
<b>DET4.WIN1.UIT1</b>	no	0..36000 (1)	TCCD Exposure time
<b>DPR.CATG</b>	yes	(CALIB)	Data Prod. Cath.
<b>DPR.TECH</b>	yes	(IMAGE)	Data Prod. Tech.
<b>DPR.TYPE</b>	yes	(FLAT,SKY)	Data Prod. Type
<b>INS.FILT1.NAME</b>	yes	u_prime g_prime r_prime i_prime z_prime U B V R I PV(B) PV(V) (V)	
G Filter			
<b>SEQ.NEXPO</b>	no	0..100 (1)	Number of exposures
Parameter	Hidden	Value	Label

Calibration template to measure the detector gain and linearity

XSHOOTER_img_cal_DetLin.tsf			
<i>To be specified:</i>			
Parameter	Hidden	Range (Default)	Label
<b>DET4.WIN1.UIT1</b>	no	0..36000 (1)	TCCD Exposure time
<b>DPR.CATG</b>	yes	(CALIB)	Data Prod. Cath.
<b>DPR.TECH</b>	yes	(IMAGE)	Data Prod. Tech.
<b>DPR.TYPE</b>	yes	(FLAT,LINEARITY,DETCHAR)	Data Prod. Type
<b>INS.FILT1.NAME</b>	no	u_prime g_prime r_prime i_prime z_prime U B V R I PV(B) PV(V) (V)	
G Filter			
<b>SEQ.EXPO.STEP</b>	no	0..3600 (1)	Exposure time step
<b>SEQ.NEXPO</b>	no	1..100 (1)	Number of exposures
<b>SEQ.NLOOP</b>	no	1..100 (2)	Number of loops (pairs)
Parameter	Hidden	Value	Label